

Qualitative Compound Report

Analysis Info


Analysis Name D:\Data\ggc\CH25_P1-D-7_01_7536.d
 Method lc_qtof_directospos.m
 Sample Name CH25
 Comment Sv: CH3CN + MeOH + HCOOH
 Uhrig

Acquisition Date 7/14/2023 3:40:39 PM

Operator ELB
 Instrument micrOTOF-Q II

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	70 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	300.0 Vpp	Set Divert Valve	Source

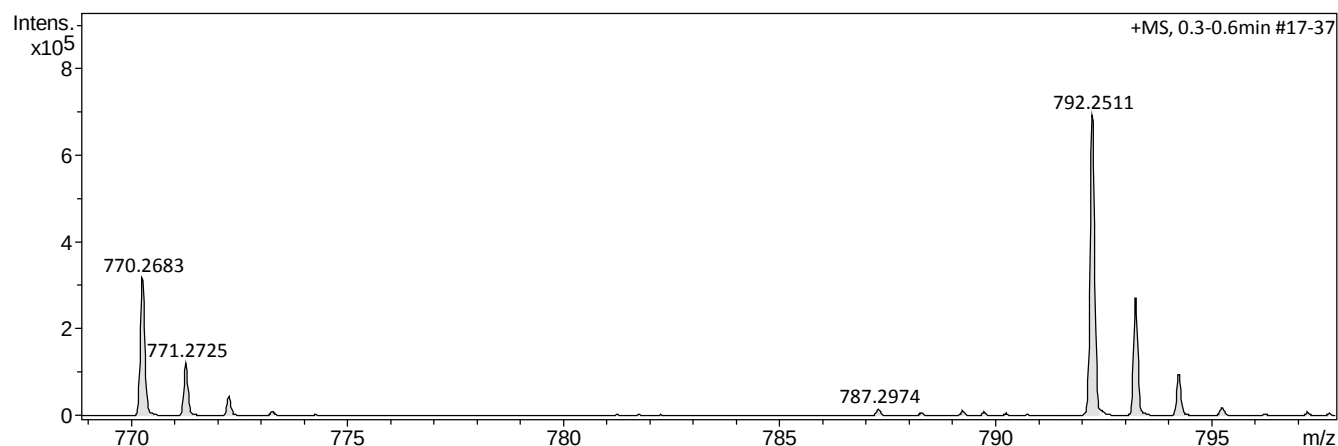

Meas. m/z	#	Ion Formula	m/z	err [ppm]	mSigma	# mSigma	Score	rdb	e ⁻ Conf	N-Rule
770.2683	1	C35H48NO16S	770.2688	0.6	12.9	1	100.00	12.5	even	ok
792.2511	1	C35H47NNaO16S	792.2508	-0.4	11.2	1	100.00	12.5	even	ok