

Qualitative Compound Report

Analysis Info


Analysis Name D:\Data\ggc\DS04 11 al 13_P1-C-1_01_8259.d
 Method lc_qtof_directospos.m
 Sample Name DS04 11 al 13
 Comment Sv: DCM + MeOH + HCOOH
 ML Uhrig

Acquisition Date 11/2/2023 1:52:08 PM

Operator ELB
 Instrument micrOTOF-Q II

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	70 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	300.0 Vpp	Set Divert Valve	Source

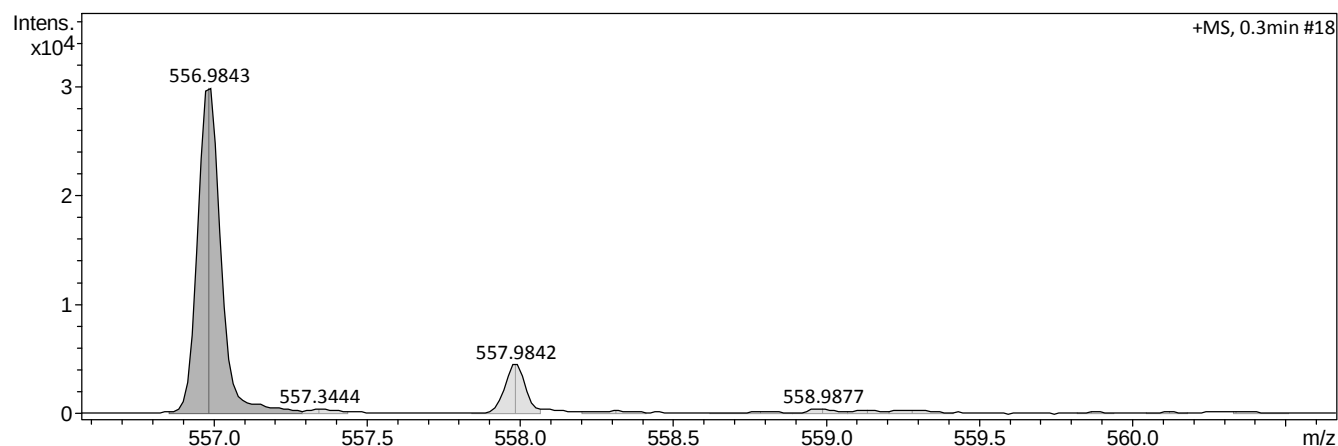

Meas. m/z	#	Ion Formula	m/z	err [ppm]	mSigma	# mSigma	Score	rdb	e ⁻ Conf	N-Rule
556.9843	1	C13H16F9INaO4	556.9842	-0.2	4.2	1	100.00	0.5	even	ok