

Qualitative Compound Report

Analysis Info


Analysis Name D:\Data\ggc\DS04 17 al 19_P1-C-2_01_8260.d
 Method lc_qtof_directospos.m
 Sample Name DS04 17 al 19
 Comment Sv: DCM + MeOH + HCOOH
 ML Uhrig

Acquisition Date 11/2/2023 1:57:14 PM

Operator ELB
 Instrument micrOTOF-Q II

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	70 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	300.0 Vpp	Set Divert Valve	Source

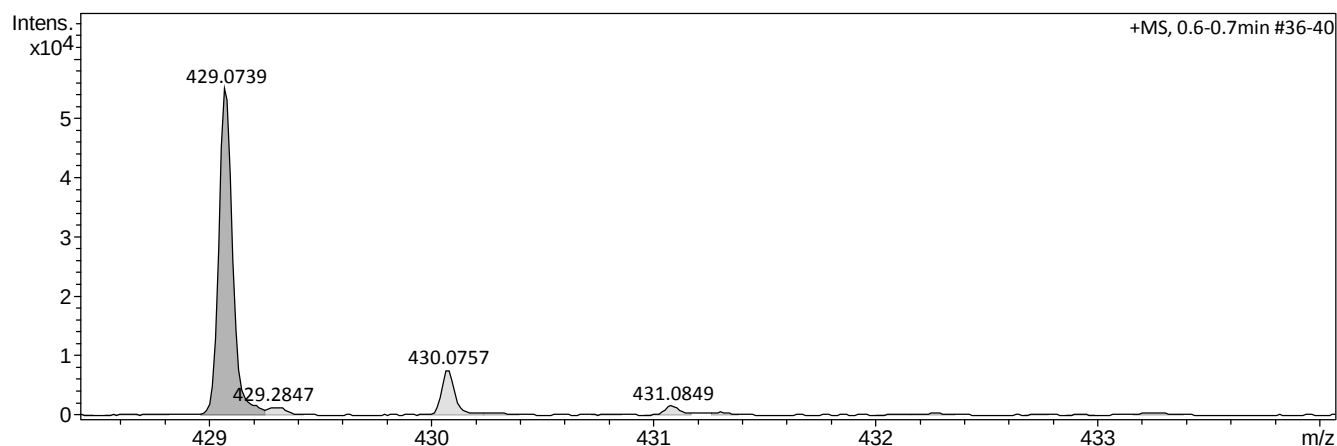

Meas. m/z	#	Ion Formula	m/z	err [ppm]	mSigma	# mSigma	Score	rdb	e ⁻ Conf	N-Rule
429.0739	1	C13H15F9NaO4	429.0719	-4.8	7.9	1	100.00	1.5	even	ok