

Qualitative Compound Report

Analysis Info

Analysis Name D:\Data\ggc\NFC-F5_P1-C-7_01_7527.d
Method lc_qtof_directospos.m
Sample Name NFC-F5
Comment Sv: DCM + MeOH + HCOOH
Uhrig


Acquisition Date 7/14/2023 2:54:36 PM

Operator ELB
Instrument micrOTOF-Q II



Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	70 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	300.0 Vpp	Set Divert Valve	Source

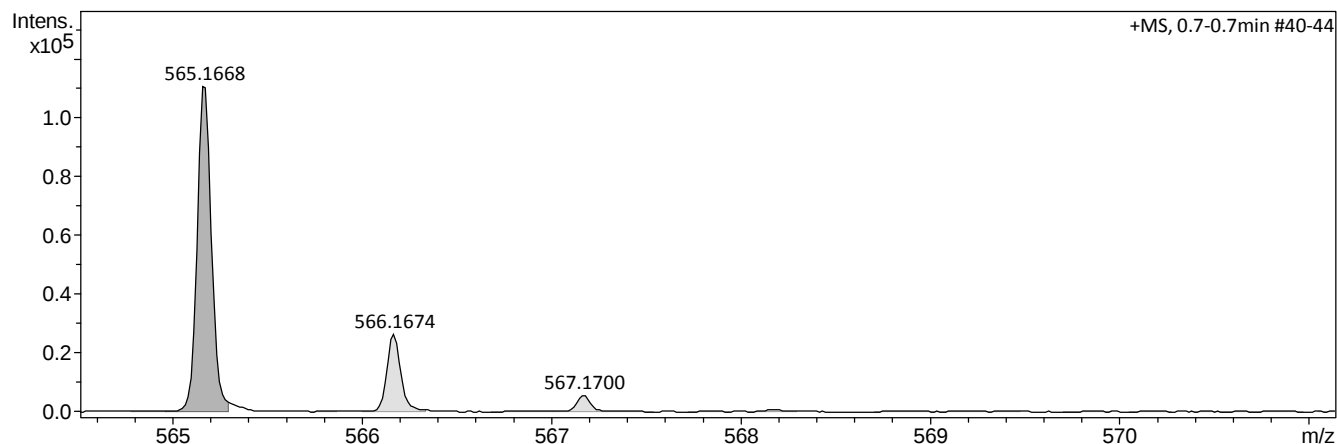

Meas. m/z	#	Ion Formula	m/z	err [ppm]	mSigma	# mSigma	Score	rdb	e ⁻ Conf	N-Rule
565.1668	1	C23H30N2NaO13	565.1640	-4.9	13.3	1	49.60	9.5	even	ok