

# Qualitative Compound Report

## Analysis Info


Analysis Name D:\Data\ggc\NFC-F6 F18-26\_P1-F-8\_01\_7287.d  
 Method lc\_qtof\_directospos.m  
 Sample Name NFC-F6 F18-26  
 Comment Sv: DCM + MeOH  
 ML Uhrig

Acquisition Date 5/30/2023 9:33:54 AM

Operator ELB  
 Instrument micrOTOF-Q II

## Acquisition Parameter

|             |            |                       |           |                  |           |
|-------------|------------|-----------------------|-----------|------------------|-----------|
| Source Type | ESI        | Ion Polarity          | Positive  | Set Nebulizer    | 3.5 Bar   |
| Focus       | Not active | Set Capillary         | 4000 V    | Set Dry Heater   | 200 °C    |
| Scan Begin  | 100 m/z    | Set End Plate Offset  | -500 V    | Set Dry Gas      | 7.0 l/min |
| Scan End    | 1500 m/z   | Set Collision Cell RF | 300.0 Vpp | Set Divert Valve | Source    |

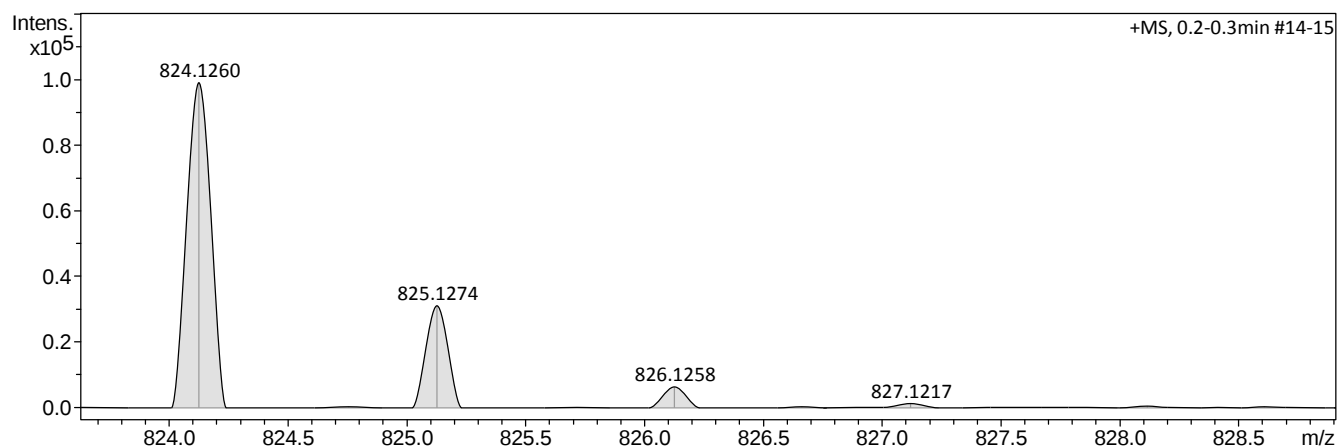

| Meas. m/z | # | Ion Formula    | m/z      | err [ppm] | mSigma | # mSigma | Score  | rdb  | e <sup>-</sup> Conf | N-Rule |
|-----------|---|----------------|----------|-----------|--------|----------|--------|------|---------------------|--------|
| 824.1260  | 1 | C30H36IN5NaO13 | 824.1247 | -1.7      | 23.1   | 1        | 100.00 | 14.5 | even                | ok     |