

Mass Spectrum List Report

Analysis Info


Analysis Name D:\Data\ggc\NFC-F7_P1-B-5_01_9015.d
 Method lc_qtof_directospos.m
 Sample Name NFC-F7
 Comment Sv: DMSO + HCOOH
 Uhrig

Acquisition Date 4/18/2024 3:38:10 PM

Operator ELB
 Instrument / Ser# microTOF-Q II

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	70 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	300.0 Vpp	Set Divert Valve	Source

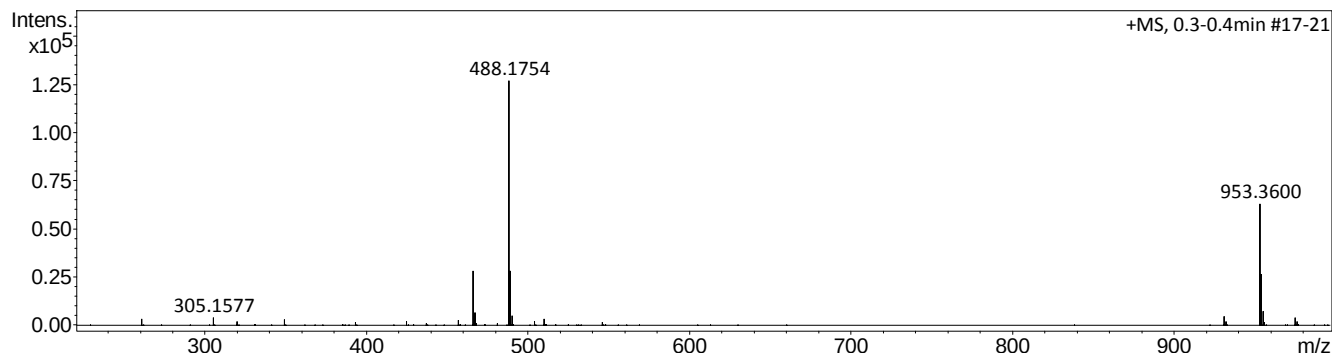

#	m/z	I	I %
1	217.1047	1908	1.5
2	261.1327	3489	2.8
3	305.1577	4019	3.2
4	320.1354	2047	1.6
5	331.2081	934	0.7
6	349.1816	2984	2.4
7	393.2112	1749	1.4
8	425.1355	2214	1.7
9	437.2351	1264	1.0
10	457.1981	2659	2.1
11	466.1923	28356	22.4
12	467.1966	6778	5.3
13	468.1981	1113	0.9
14	473.3459	786	0.6
15	481.2650	968	0.8
16	488.1754	126716	100.0
17	489.1794	28086	22.2
18	490.1804	4947	3.9
19	491.1831	853	0.7
20	504.1500	1993	1.6
21	510.1622	3292	2.6
22	546.1324	1826	1.4
23	931.3738	4772	3.8
24	932.3819	2160	1.7
25	953.3600	62855	49.6
26	954.3626	26401	20.8
27	955.3612	7510	5.9
28	956.3590	1894	1.5
29	975.3408	4068	3.2
30	976.3368	2093	1.7