

Mass Spectrum List Report

Analysis Info


Analysis Name D:\Data\ggc\pm-1-131000001.d
 Method tunelow300924.m
 Sample Name pm-1-131
 Comment Sv: DCM + MeOH
 Uhrig

Acquisition Date 10/29/2024 11:54:20 AM

Operator EB - MV
 Instrument / Ser# microTOF-Q

Acquisition Parameter

Source Type	APCI	Ion Polarity	Positive	Set Nebulizer	1.6 Bar
Focus	Not active	Set Capillary	4500 V	Set Dry Heater	200 °C
Scan Begin	100 m/z	Set End Plate Offset	-500 V	Set Dry Gas	8.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	250.0 Vpp	Set Divert Valve	Source

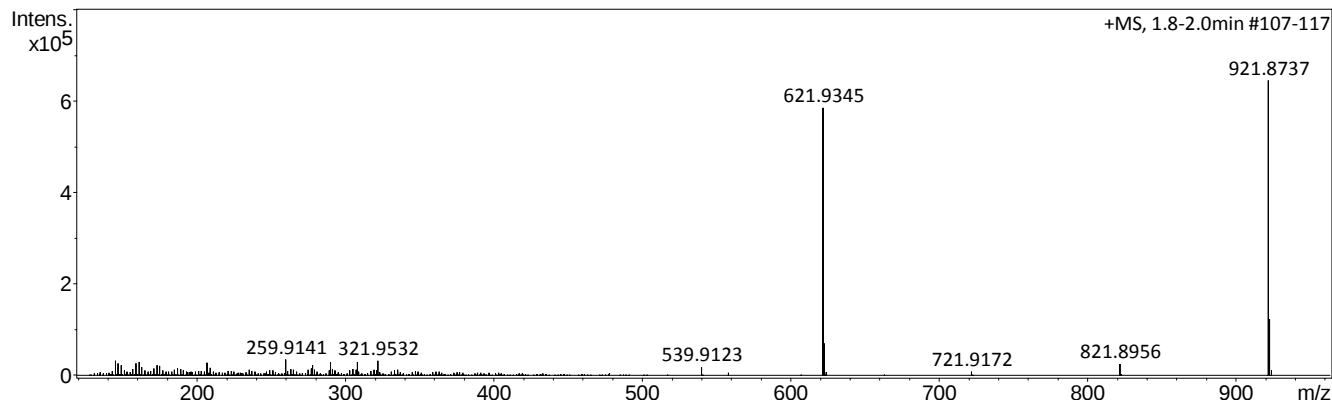

#	m/z	I	I %
1	144.9975	32356	5.0
2	147.0096	27048	4.2
3	149.0196	22864	3.6
4	156.9979	14604	2.3
5	159.0115	26725	4.2
6	161.0235	29713	4.6
7	163.0288	18472	2.9
8	171.0120	16304	2.5
9	173.0243	22820	3.5
10	175.0374	21758	3.4
11	187.0358	15323	2.4
12	189.0490	14628	2.3
13	206.9956	28082	4.4
14	209.0288	17072	2.7
15	235.0777	13574	2.1
16	259.9141	35165	5.5
17	263.1081	14435	2.2
18	277.1219	15881	2.5
19	277.9243	23100	3.6
20	289.9262	30260	4.7
21	291.1366	15066	2.3
22	305.1511	14670	2.3
23	307.9363	30276	4.7
24	321.9532	31992	5.0
25	539.9123	18133	2.8
26	621.9345	584200	90.8
27	622.9372	70502	11.0
28	821.8956	26074	4.1
29	921.8737	643523	100.0
30	922.8769	122509	19.0