

Mass Spectrum List Report

Analysis Info


Analysis Name D:\Data\24-060401_P1-C-1_01_9596.d
Method vallejo 281024.m
Sample Name 24-060401
Comment CnFnCol
Sv: Agua
Vallejo - UNC

Acquisition Date 28/10/2024 2:24:03 p. m.

Operator EB - MV
Instrument / Ser# microTOF-Q

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	2.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	90 m/z	Set End Plate Offset	-500 V	Set Dry Gas	11.0 l/min
Scan End	1500 m/z	Set Collision Cell RF	250.0 Vpp	Set Divert Valve	Source

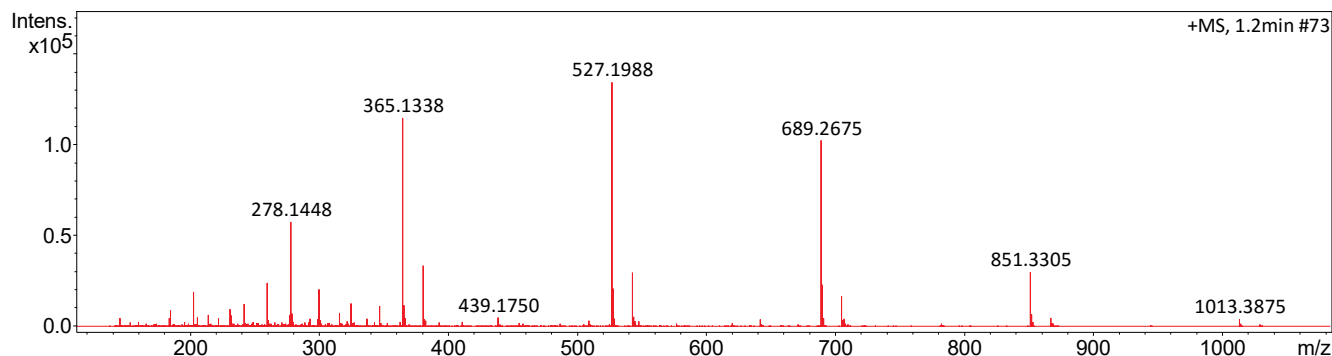

#	m/z	I	I %
1	185.0568	9042	6.7
2	203.0687	18920	14.1
3	206.0639	5088	3.8
4	214.1249	6466	4.8
5	222.0365	4844	3.6
6	231.1515	9734	7.3
7	232.1369	6018	4.5
8	242.1213	12442	9.3
9	260.1321	24155	18.0
10	277.1136	6406	4.8
11	278.1448	57459	42.8
12	279.1478	7194	5.4
13	300.1296	20343	15.2
14	316.1055	7477	5.6
15	325.1375	12798	9.5
16	347.1222	11432	8.5
17	365.1338	114689	85.5
18	366.1357	11804	8.8
19	381.1078	33406	24.9
20	439.1750	4956	3.7
21	527.1988	134132	100.0
22	528.2039	20754	15.5
23	543.1747	29654	22.1
24	544.1779	5405	4.0
25	689.2675	102247	76.2
26	690.2686	22958	17.1
27	705.2444	16439	12.3
28	851.3305	30031	22.4
29	852.3355	6859	5.1
30	867.3008	4826	3.6