

# Mass Spectrum List Report

## Analysis Info

Analysis Name D:\Data\24-060401\_P1-C-1\_01\_9596.d  
 Method vallejo 281024.m  
 Sample Name 24-060401  
 Comment CnFnCol  
 Sv: Agua  
 Vallejo - UNC


Acquisition Date 28/10/2024 2:24:03 p. m.

Operator EB - MV

Instrument / Ser# microTOF-Q

## Acquisition Parameter

|             |            |                       |           |                  |            |
|-------------|------------|-----------------------|-----------|------------------|------------|
| Source Type | ESI        | Ion Polarity          | Positive  | Set Nebulizer    | 2.5 Bar    |
| Focus       | Not active | Set Capillary         | 4000 V    | Set Dry Heater   | 200 °C     |
| Scan Begin  | 90 m/z     | Set End Plate Offset  | -500 V    | Set Dry Gas      | 11.0 l/min |
| Scan End    | 1500 m/z   | Set Collision Cell RF | 250.0 Vpp | Set Divert Valve | Source     |

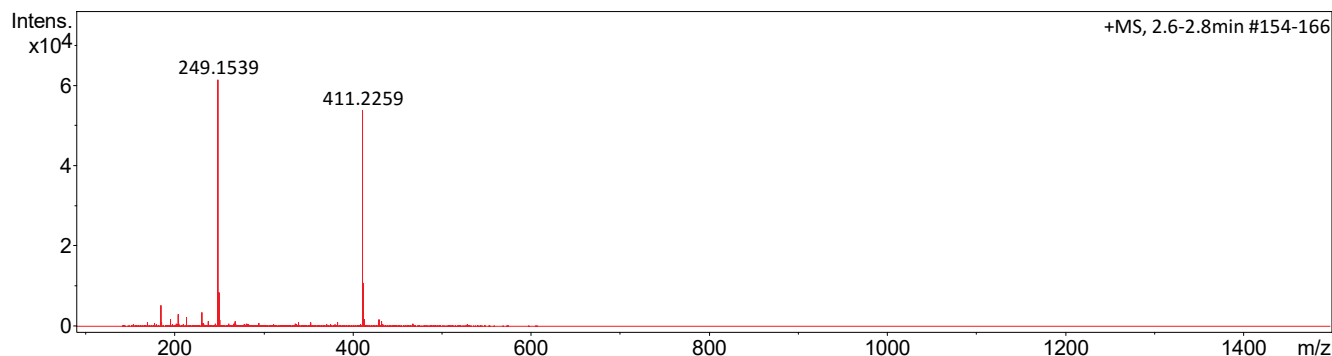

| #  | m/z      | I     | I %   |
|----|----------|-------|-------|
| 1  | 170.0695 | 1027  | 1.7   |
| 2  | 178.0975 | 802   | 1.3   |
| 3  | 185.1296 | 5211  | 8.5   |
| 4  | 186.1276 | 993   | 1.6   |
| 5  | 196.0526 | 1723  | 2.8   |
| 6  | 202.0775 | 646   | 1.1   |
| 7  | 204.1248 | 2991  | 4.9   |
| 8  | 205.1307 | 662   | 1.1   |
| 9  | 214.0674 | 2223  | 3.6   |
| 10 | 231.1402 | 3552  | 5.8   |
| 11 | 232.1222 | 877   | 1.4   |
| 12 | 238.1053 | 1359  | 2.2   |
| 13 | 246.1515 | 720   | 1.2   |
| 14 | 249.1539 | 61417 | 100.0 |
| 15 | 250.1574 | 8387  | 13.7  |
| 16 | 251.1566 | 1708  | 2.8   |
| 17 | 261.1484 | 707   | 1.2   |
| 18 | 267.1725 | 723   | 1.2   |
| 19 | 268.1486 | 1358  | 2.2   |
| 20 | 281.1411 | 718   | 1.2   |
| 21 | 295.1574 | 862   | 1.4   |
| 22 | 339.1601 | 949   | 1.5   |
| 23 | 353.1470 | 1064  | 1.7   |
| 24 | 383.1460 | 1039  | 1.7   |
| 25 | 411.2259 | 53791 | 87.6  |
| 26 | 412.2269 | 10855 | 17.7  |
| 27 | 413.2279 | 1828  | 3.0   |
| 28 | 430.2169 | 1793  | 2.9   |
| 29 | 433.2075 | 1385  | 2.3   |
| 30 | 468.2072 | 633   | 1.0   |