

Mass Spectrum List Report

Analysis Info


Analysis Name D:\Data\24-060401_P1-C-1_01_9596.d
 Method vallejo 281024.m
 Sample Name 24-060401
 Comment CnFnCol
 Sv: Agua
 Vallejo - UNC

Acquisition Date 28/10/2024 2:24:03 p. m.

Operator EB - MV
 Instrument / Ser# microTOF-Q

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	2.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	90 m/z	Set End Plate Offset	-500 V	Set Dry Gas	11.0 l/min
Scan End	1500 m/z	Set Collision Cell RF	250.0 Vpp	Set Divert Valve	Source

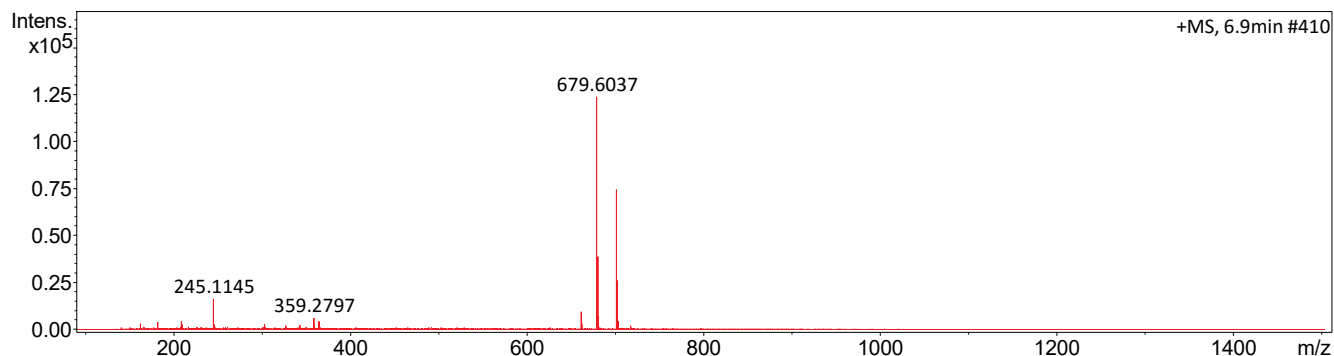

#	m/z	I	I %
1	163.0624	3244	2.6
2	178.1053	1254	1.0
3	182.1753	4071	3.3
4	208.1221	1329	1.1
5	209.1886	4408	3.6
6	210.1716	2797	2.3
7	217.1214	1324	1.1
8	245.1145	16513	13.4
9	246.1214	2696	2.2
10	247.1349	1271	1.0
11	261.1239	1535	1.2
12	301.1482	1279	1.0
13	303.1610	2908	2.4
14	327.1980	2046	1.7
15	343.1966	2374	1.9
16	343.3495	1982	1.6
17	350.2661	1374	1.1
18	359.2797	6147	5.0
19	359.7816	2088	1.7
20	365.1740	4558	3.7
21	366.1822	1273	1.0
22	661.5899	9615	7.8
23	662.5978	3011	2.4
24	679.6037	123589	100.0
25	680.6065	38984	31.5
26	681.6052	6913	5.6
27	701.5876	74319	60.1
28	702.5913	26198	21.2
29	703.5942	4422	3.6
30	717.5560	2183	1.8