

Mass Spectrum List Report

Analysis Info


Analysis Name D:\Data\24-060401_P1-C-1_01_9596.d
Method vallejo 281024.m
Sample Name 24-060401
Comment CnFnCol
Sv: Agua
Vallejo - UNC

Acquisition Date 28/10/2024 2:24:03 p. m.

Operator EB - MV
Instrument / Ser# microTOF-Q

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	2.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	90 m/z	Set End Plate Offset	-500 V	Set Dry Gas	11.0 l/min
Scan End	1500 m/z	Set Collision Cell RF	250.0 Vpp	Set Divert Valve	Source

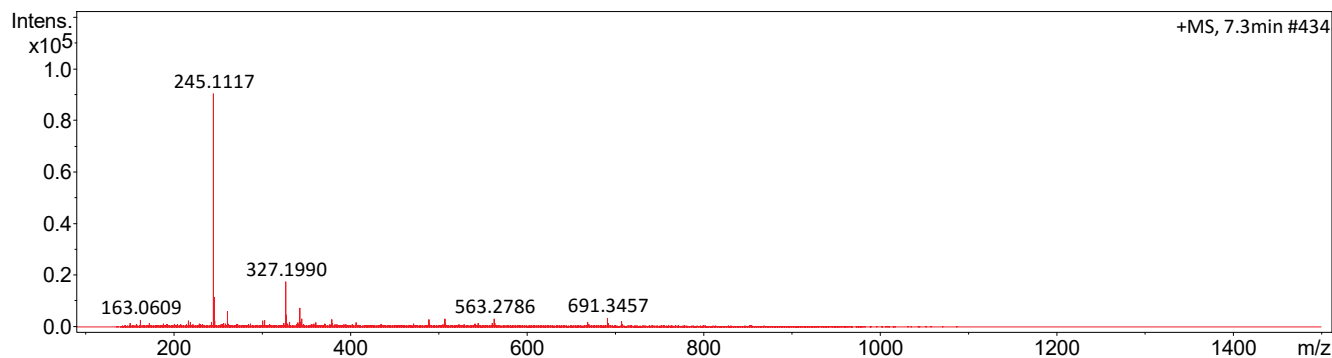

#	m/z	I	I %
1	151.0600	1586	1.8
2	163.0609	2666	3.0
3	173.1133	1646	1.8
4	217.1146	2544	2.8
5	219.0974	1784	2.0
6	243.1088	1675	1.9
7	245.1117	90269	100.0
8	246.1158	11562	12.8
9	247.1224	2504	2.8
10	257.1217	1609	1.8
11	261.1104	6349	7.0
12	301.1468	2430	2.7
13	303.1587	2811	3.1
14	327.1990	17608	19.5
15	328.1996	4760	5.3
16	331.1968	1996	2.2
17	341.1896	1896	2.1
18	343.1929	7589	8.4
19	344.1942	1984	2.2
20	345.2055	3309	3.7
21	361.2037	1896	2.1
22	379.2159	2908	3.2
23	407.1866	1859	2.1
24	489.2676	2972	3.3
25	507.2822	3286	3.6
26	545.2704	1527	1.7
27	563.2786	3338	3.7
28	669.3566	2101	2.3
29	691.3457	3608	4.0
30	707.3387	2323	2.6