

Mass Spectrum List Report

Analysis Info


Analysis Name D:\Data\24-060401_P1-C-1_01_9596.d
Method vallejo 281024.m
Sample Name 24-060401
Comment CnFnCol
Sv: Agua
Vallejo - UNC

Acquisition Date 28/10/2024 2:24:03 p. m.

Operator EB - MV
Instrument / Ser# micrOTOF-Q

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	2.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	90 m/z	Set End Plate Offset	-500 V	Set Dry Gas	11.0 l/min
Scan End	1500 m/z	Set Collision Cell RF	250.0 Vpp	Set Divert Valve	Source

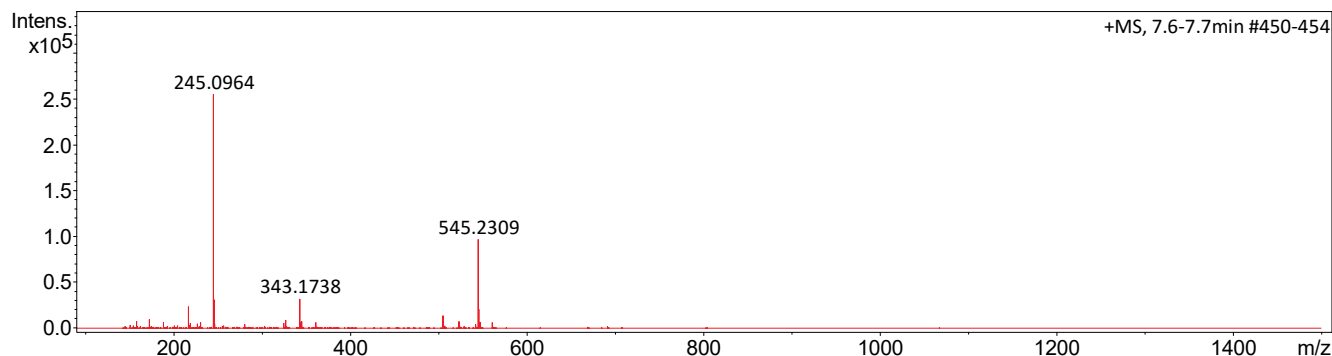

#	m/z	I	I %
1	151.0491	3479	1.4
2	158.0803	7872	3.1
3	173.1046	10110	4.0
4	189.0930	6211	2.4
5	201.1022	3252	1.3
6	205.0647	3290	1.3
7	217.0989	23880	9.4
8	218.1017	3633	1.4
9	219.0804	6059	2.4
10	227.0864	5308	2.1
11	231.0811	6735	2.6
12	245.0964	254567	100.0
13	246.0992	31627	12.4
14	247.1049	5263	2.1
15	257.1007	2949	1.2
16	281.1085	4493	1.8
17	325.1606	5664	2.2
18	327.1745	9264	3.6
19	343.1738	32126	12.6
20	344.1746	6737	2.6
21	345.1878	7704	3.0
22	361.1866	6751	2.7
23	505.2322	14021	5.5
24	506.2397	3741	1.5
25	523.2462	8036	3.2
26	542.2245	4527	1.8
27	545.2309	97239	38.2
28	546.2350	20914	8.2
29	547.2432	7221	2.8
30	561.2093	6220	2.4