

Mass Spectrum List Report

Analysis Info


Analysis Name D:\Data\24-060401_P1-C-1_01_9596.d
 Method vallejo 281024.m
 Sample Name 24-060401
 Comment CnFnCol
 Sv: Agua
 Vallejo - UNC

Acquisition Date 28/10/2024 2:24:03 p. m.

Operator EB - MV
 Instrument / Ser# microTOF-Q

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	2.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	90 m/z	Set End Plate Offset	-500 V	Set Dry Gas	11.0 l/min
Scan End	1500 m/z	Set Collision Cell RF	250.0 Vpp	Set Divert Valve	Source

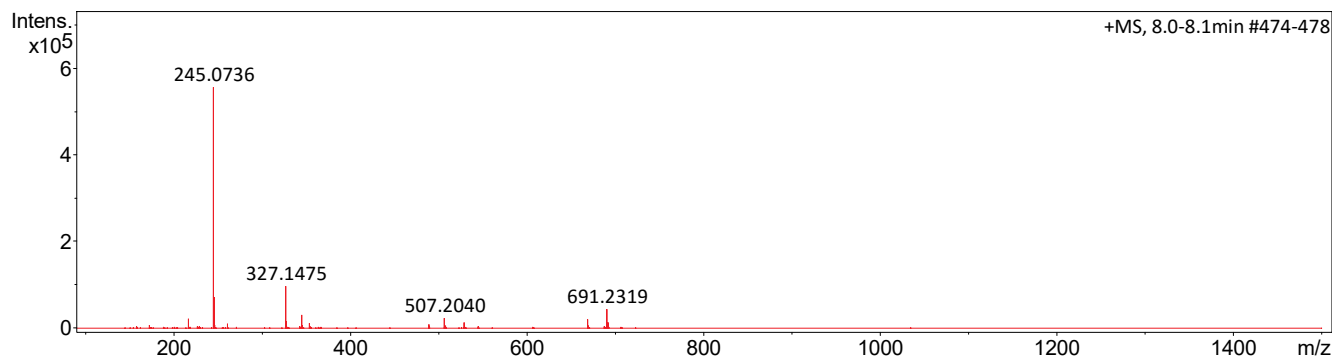

#	m/z	I	I %
1	158.0666	4560	0.8
2	173.0887	7672	1.4
3	189.0763	3580	0.6
4	217.0778	21762	3.9
5	227.0648	4472	0.8
6	229.0787	4665	0.8
7	245.0736	556096	100.0
8	246.0759	73002	13.1
9	247.0793	7922	1.4
10	261.0672	10160	1.8
11	327.1475	96980	17.4
12	328.1508	16958	3.0
13	343.1403	3877	0.7
14	345.1560	31149	5.6
15	346.1576	6197	1.1
16	354.1032	11989	2.2
17	354.6036	4256	0.8
18	489.1975	9581	1.7
19	507.2040	23632	4.2
20	508.2090	5651	1.0
21	529.1856	13575	2.4
22	530.1913	3259	0.6
23	545.1723	4874	0.9
24	669.2526	20583	3.7
25	670.2511	6069	1.1
26	688.2244	4707	0.8
27	688.7252	3297	0.6
28	691.2319	44747	8.0
29	692.2328	14090	2.5
30	707.2080	3753	0.7