

Qualitative Compound Report

Analysis Info


Analysis Name D:\Data\ggc\25-020501_P1-E-1_01_10049.d
 Method lc_ms directos tunelow300924.m
 Sample Name 25-020501
 Comment DopaOSilPropBr
 Sv: DCM + MeOH + HCOOH
 Oscar Varela

Acquisition Date 2/21/2025 9:55:16 AM

Operator EB - MV
 Instrument micrOTOF-Q

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	2.0 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	100 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1200 m/z	Set Collision Cell RF	250.0 Vpp	Set Divert Valve	Source

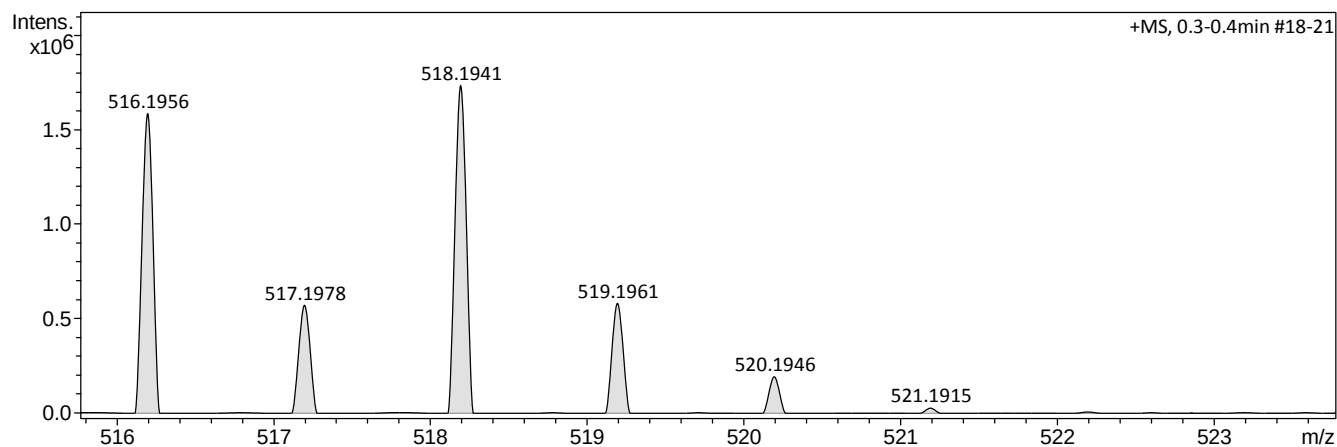

Meas. m/z	#	Ion Formula	m/z	err [ppm]	mSigma	# mSigma	Score	rdb	e ⁻ Conf	N-Rule
516.1956	1	C23H43BrNO3Si2	516.1959	0.6	9.1	1	100.00	4.5	even	ok