

Qualitative Compound Report

Analysis Info


Analysis Name D:\Data\ggc\25-020507_P1-E-7_01_10055.d
 Method lc_ms directos tunelow300924.m
 Sample Name 25-020507
 Comment 4OMsNHexil
 Sv: DCM + MeOH + HCOOH
 Oscar Varela

Acquisition Date 2/21/2025 10:31:19 AM

Operator EB - MV
 Instrument micrOTOF-Q

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	2.0 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	100 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1200 m/z	Set Collision Cell RF	250.0 Vpp	Set Divert Valve	Source

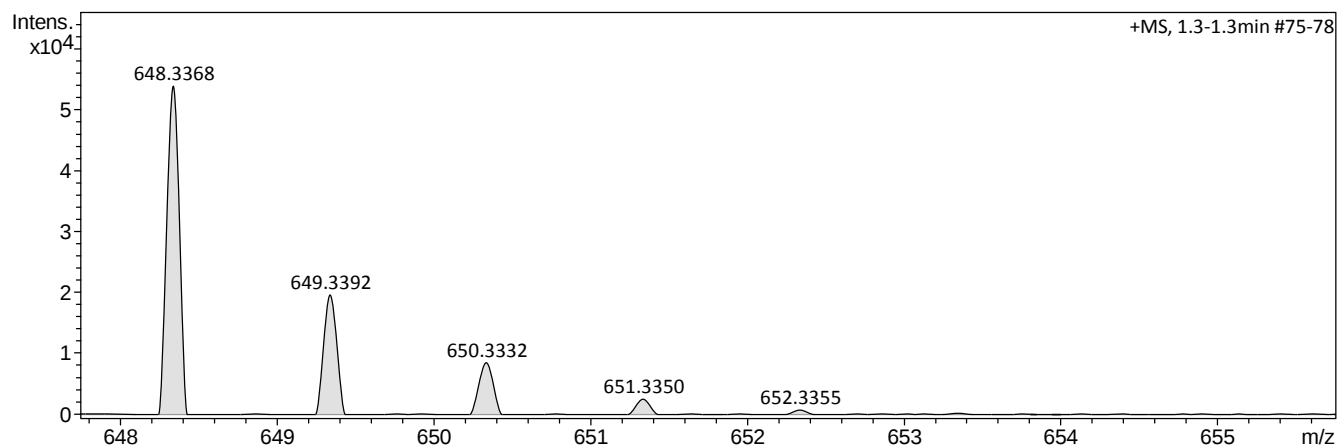

Meas. m/z	#	Ion Formula	m/z	err [ppm]	mSigma	# mSigma	Score	rdb	e ⁻ Conf	N-Rule
648.3368	1	C28H59NNaO8SSi2	648.3392	3.7	39.2	1	100.00	1.5	even	ok