

Qualitative Compound Report

Analysis Info


Analysis Name D:\Data\ggc\4OMsEt2OTBS_P1-D-8_01_8737.d
 Method lc_qtof_directospos.m
 Sample Name 4OMsEt2OTBS
 Comment Sv: DCM + HCOOH
 Varela

Acquisition Date 3/18/2024 4:50:06 PM

Operator ELB
 Instrument micrOTOF-Q II

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	70 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	300.0 Vpp	Set Divert Valve	Source

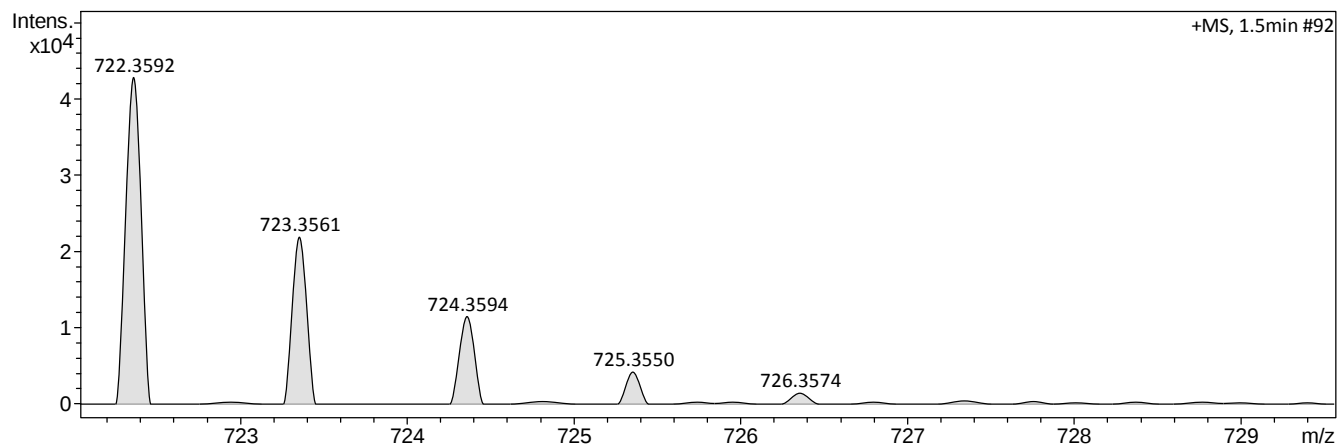

Meas. m/z	#	Ion Formula	m/z	err [ppm]	mSigma	# mSigma	Score	rdb	e ⁻ Conf	N-Rule
722.3592	1	C30H65NNaO9SSi3	722.3580	-1.6	8.2	1	100.00	1.5	even	ok