

Qualitative Compound Report

Analysis Info


Analysis Name D:\Data\ggc\4OMsNHexil6OTBS_P1-D-3_01_9807.d
 Method lc_ms directos tunelow300924.m
 Sample Name 4OMsNHexil6OTBS
 Comment Sv: DCM + MeOH + HCOOH
 Oscar Varela

Acquisition Date 12/5/2024 2:25:09 PM

Operator EB - MV
 Instrument micrOTOF-Q

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	2.0 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	100 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	250.0 Vpp	Set Divert Valve	Source

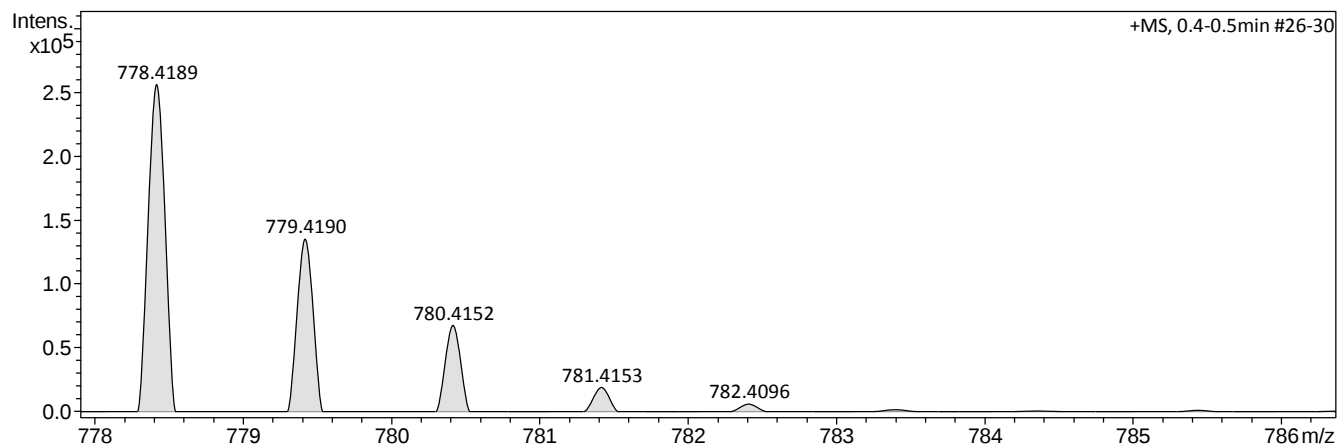

Meas. m/z	#	Ion Formula	m/z	err [ppm]	mSigma	# mSigma	Score	rdb	e ⁻ Conf	N-Rule
778.4189	1	C34H73NNaO9SSi3	778.4206	2.2	26.7	2	41.46	1.5	even	ok