

Mass Spectrum List Report

Analysis Info

Analysis Name D:\Data\ggc\4OMsNHexil_P1-D-2_01_9806.d
 Method lc_ms directos tunelow300924.m
 Sample Name 4OMsNHexil
 Comment Sv: DCM + MeOH + HCOOH
 Oscar Varela


Acquisition Date 12/5/2024 2:20:02 PM

Operator EB - MV

Instrument / Ser# microTOF-Q

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	2.0 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	100 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	250.0 Vpp	Set Divert Valve	Source

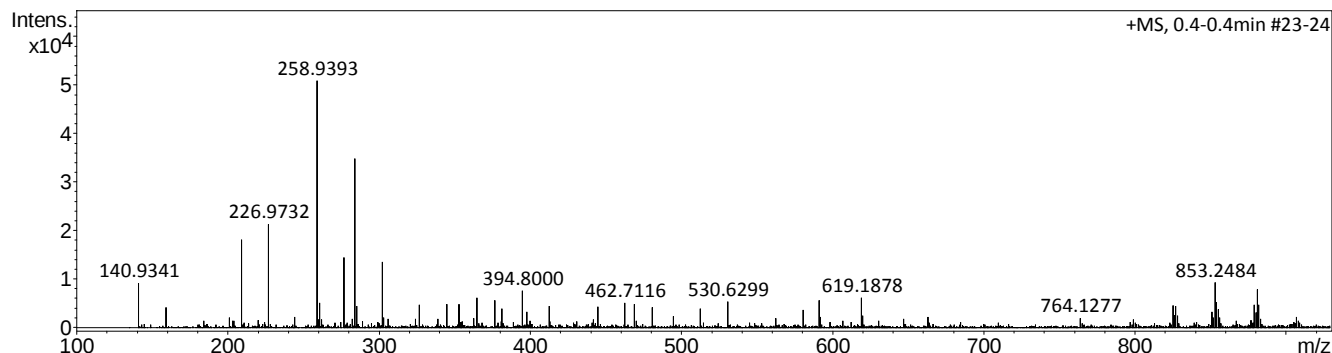

#	m/z	I	I %
1	140.9341	9233	18.2
2	158.9625	4209	8.3
3	208.9696	18118	35.7
4	226.9732	21242	41.8
5	258.9393	50801	100.0
6	260.9353	5128	10.1
7	276.9326	14387	28.3
8	284.1423	34813	68.5
9	285.1440	4483	8.8
10	302.1393	13467	26.5
11	326.8772	4741	9.3
12	344.8662	4807	9.5
13	353.2022	4832	9.5
14	365.0298	6137	12.1
15	376.8128	5599	11.0
16	394.8000	7635	15.0
17	412.7823	4440	8.7
18	444.7293	4343	8.5
19	462.7116	5085	10.0
20	469.0556	4856	9.6
21	530.6299	5382	10.6
22	591.1838	5639	11.1
23	619.1878	6149	12.1
24	825.2240	4644	9.1
25	827.2330	4474	8.8
26	853.2484	9319	18.3
27	854.2525	5226	10.3
28	879.2472	4726	9.3
29	881.2623	7876	15.5
30	882.2663	4698	9.2