

Qualitative Compound Report

Analysis Info


Analysis Name D:\Data\ggc\D-3D_P1-D-1_01_9211.d
 Method lc_qtof_directospos.m
 Sample Name D-3D
 Comment Sv: MeOH + HCOOH
 Varela

Acquisition Date 5/29/2024 3:02:53 PM

Operator MV
 Instrument micrOTOF-Q II

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	70 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	300.0 Vpp	Set Divert Valve	Source

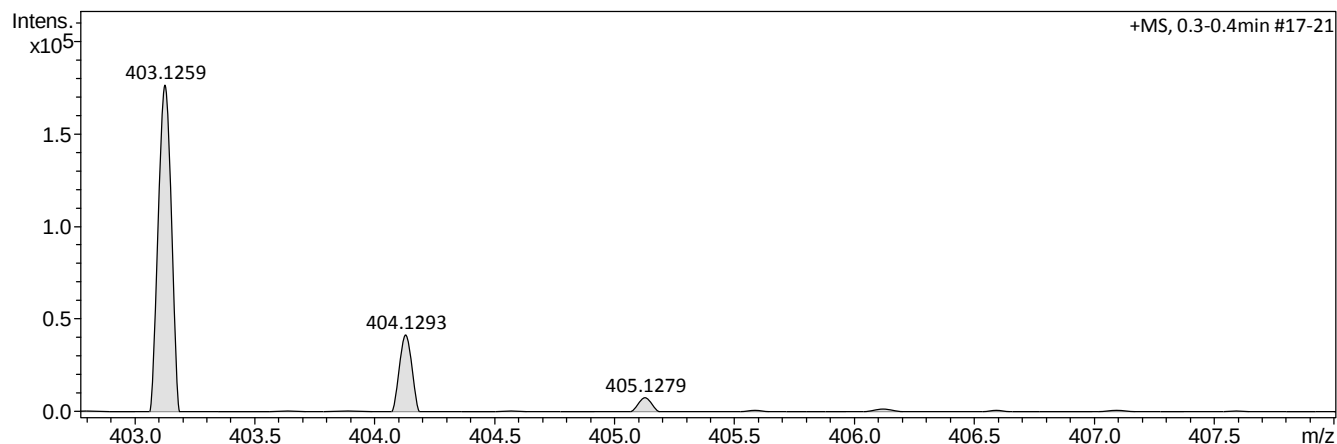

Meas. m/z	#	Ion Formula	m/z	err [ppm]	mSigma	# mSigma	Score	rdB	e ⁻ Conf	N-Rule
403.1259	1	C20H19DNO8	403.1246	-3.2	5.9	2	56.77	11.5	even	ok