

Qualitative Compound Report

Analysis Info


Analysis Name D:\Data\ggc\DopaOBnValSAc_P1-E-3_01_8741.d
 Method lc_qtof_directospos.m
 Sample Name DopaOBnValSAc
 Comment Sv: DCM + HCOOH
 Varela

Acquisition Date 3/18/2024 5:10:33 PM

Operator ELB
 Instrument micrOTOF-Q II

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	70 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	300.0 Vpp	Set Divert Valve	Source

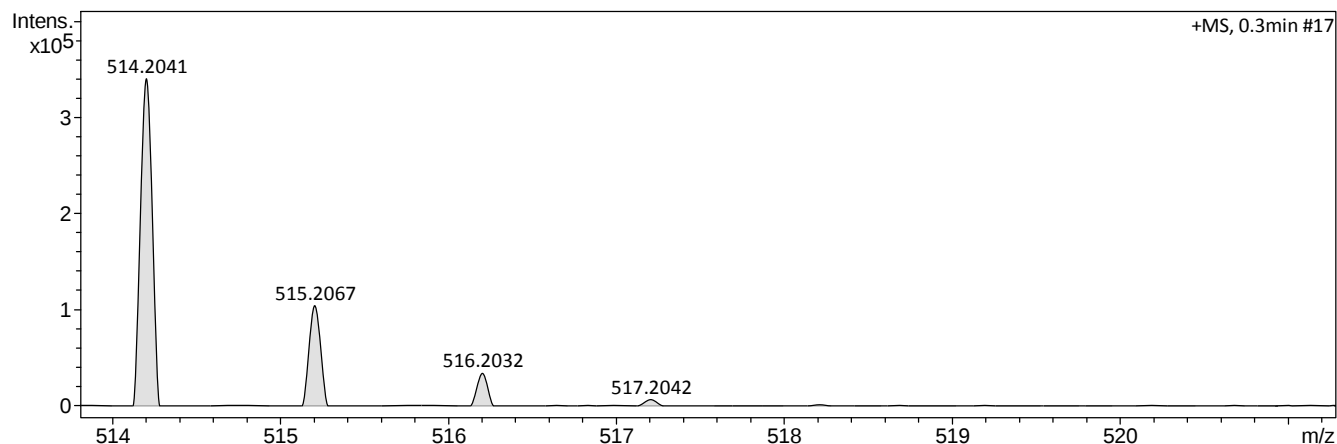

Meas. m/z	#	Ion Formula	m/z	err [ppm]	mSigma	# mSigma	Score	rdB	e ⁻ Conf	N-Rule
514.2041	1	C29H33NNaO4S	514.2023	-3.6	12.6	1	100.00	13.5	even	ok