

Qualitative Compound Report

Analysis Info


Analysis Name D:\Data\ggc\LactNHxil6OHLIBRE_P1-B-4_01_9223.d
 Method lc_qtof_directospos.m
 Sample Name LactNHxil6OHLIBRE
 Comment Sv: H2O + HCOOH
 Varela

Acquisition Date 6/5/2024 3:11:23 PM

Operator MV
 Instrument micrOTOF-Q II

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	70 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	300.0 Vpp	Set Divert Valve	Source

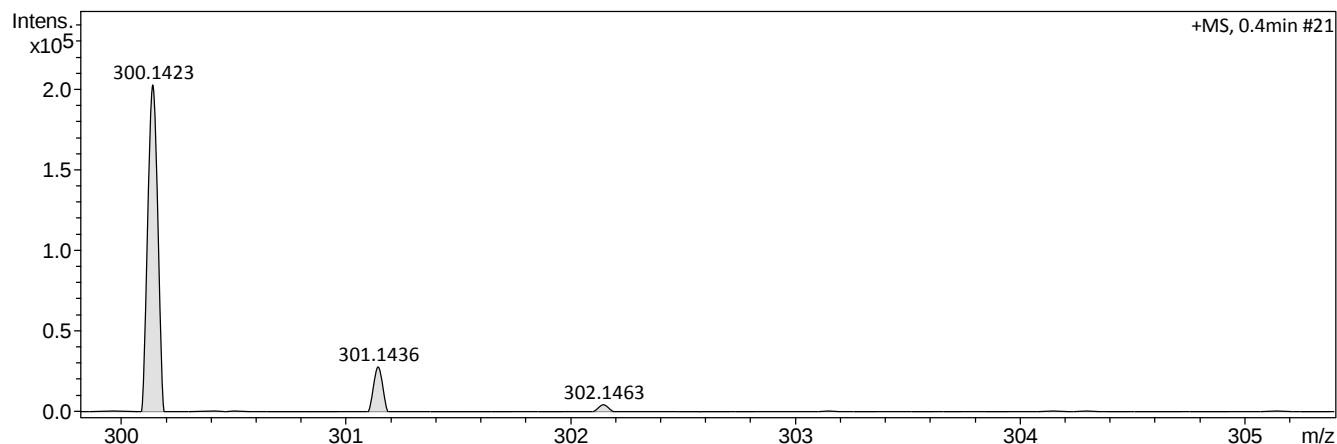

Meas. m/z	#	Ion Formula	m/z	err [ppm]	mSigma	# mSigma	Score	rdb	e ⁻ Conf	N-Rule
300.1423	1	C12H23NNaO6	300.1418	-1.8	0.8	1	100.00	1.5	even	ok