

Mass Spectrum List Report

Analysis Info

Analysis Name D:\Data\ggc\LactNHexil6OTBS_P1-D-5_01_9809.d
 Method lc_ms directos tunelow300924.m
 Sample Name LactNHexil6OTBS
 Comment Sv: DCM + MeOH + HCOOH
 Oscar Varela


Acquisition Date 12/5/2024 2:35:23 PM

Operator EB - MV

Instrument / Ser# microTOF-Q

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	2.0 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	100 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	250.0 Vpp	Set Divert Valve	Source

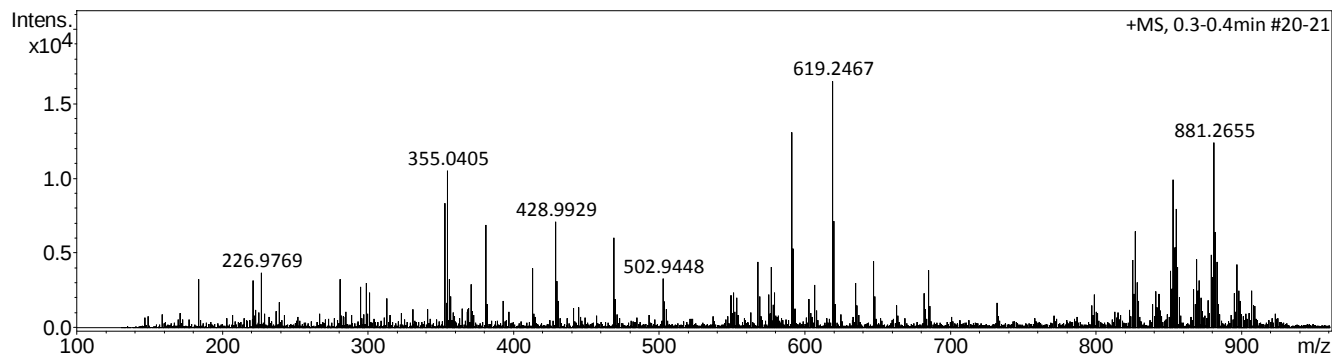

#	m/z	I	I %
1	226.9769	3688	22.4
2	353.2350	8336	50.7
3	355.0405	10481	63.7
4	381.2446	6881	41.8
5	413.1853	3976	24.2
6	428.9929	7067	42.9
7	469.1093	6015	36.6
8	502.9448	3302	20.1
9	568.1200	4394	26.7
10	577.2744	4066	24.7
11	591.2486	13050	79.3
12	592.2520	5284	32.1
13	619.2467	16458	100.0
14	620.2490	7141	43.4
15	647.2504	4423	26.9
16	685.0971	3857	23.4
17	825.2430	4542	27.6
18	827.2600	6425	39.0
19	851.2415	3806	23.1
20	853.2581	9904	60.2
21	854.2611	5385	32.7
22	855.2719	7948	48.3
23	856.2714	4033	24.5
24	869.2292	4553	27.7
25	879.2520	4858	29.5
26	880.2613	3350	20.4
27	881.2655	12351	75.0
28	882.2704	6381	38.8
29	883.2771	4396	26.7
30	897.2299	4213	25.6